

PRODUCT DISPLAY





PRODUCT SIZE



PRODUCT DETAILS



PRODUCT PHOTOGRAPH

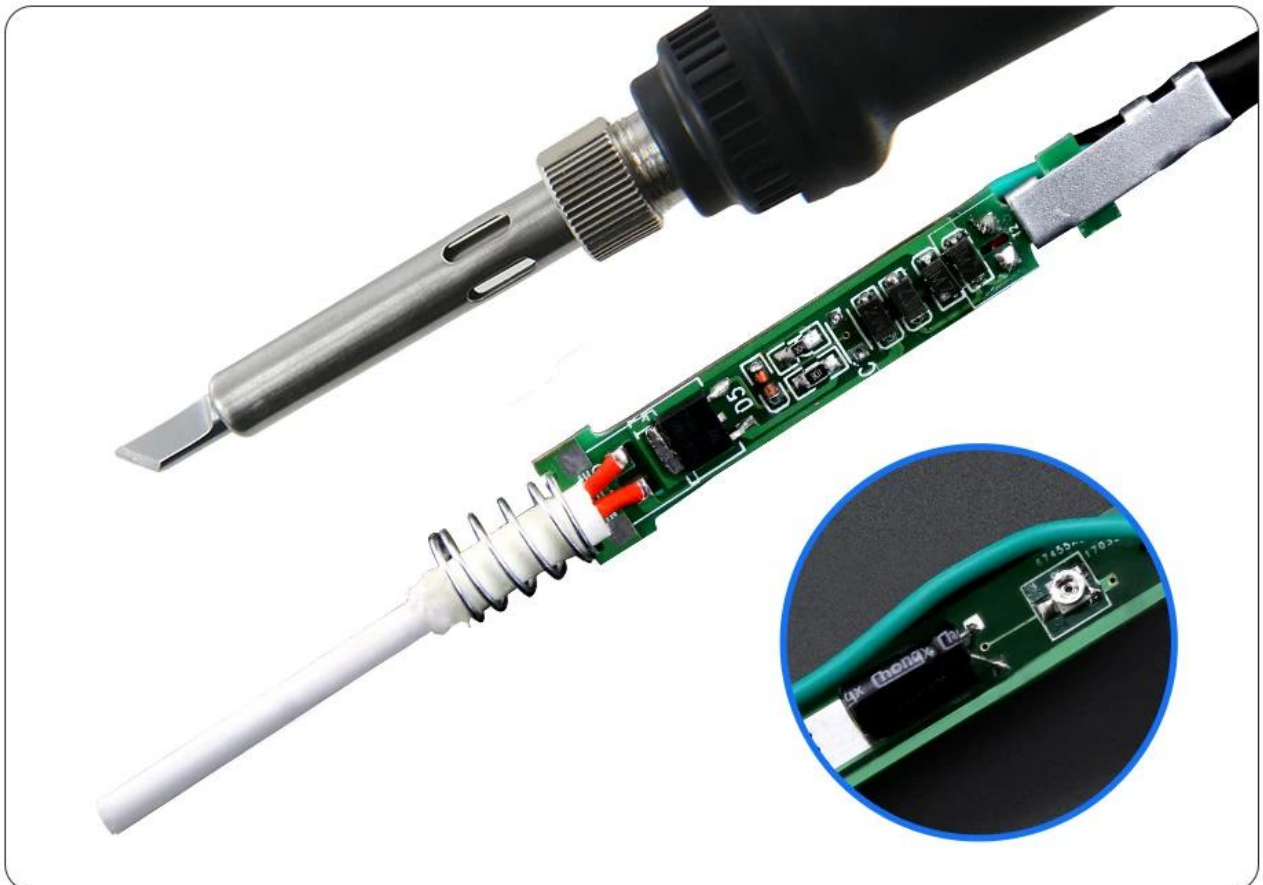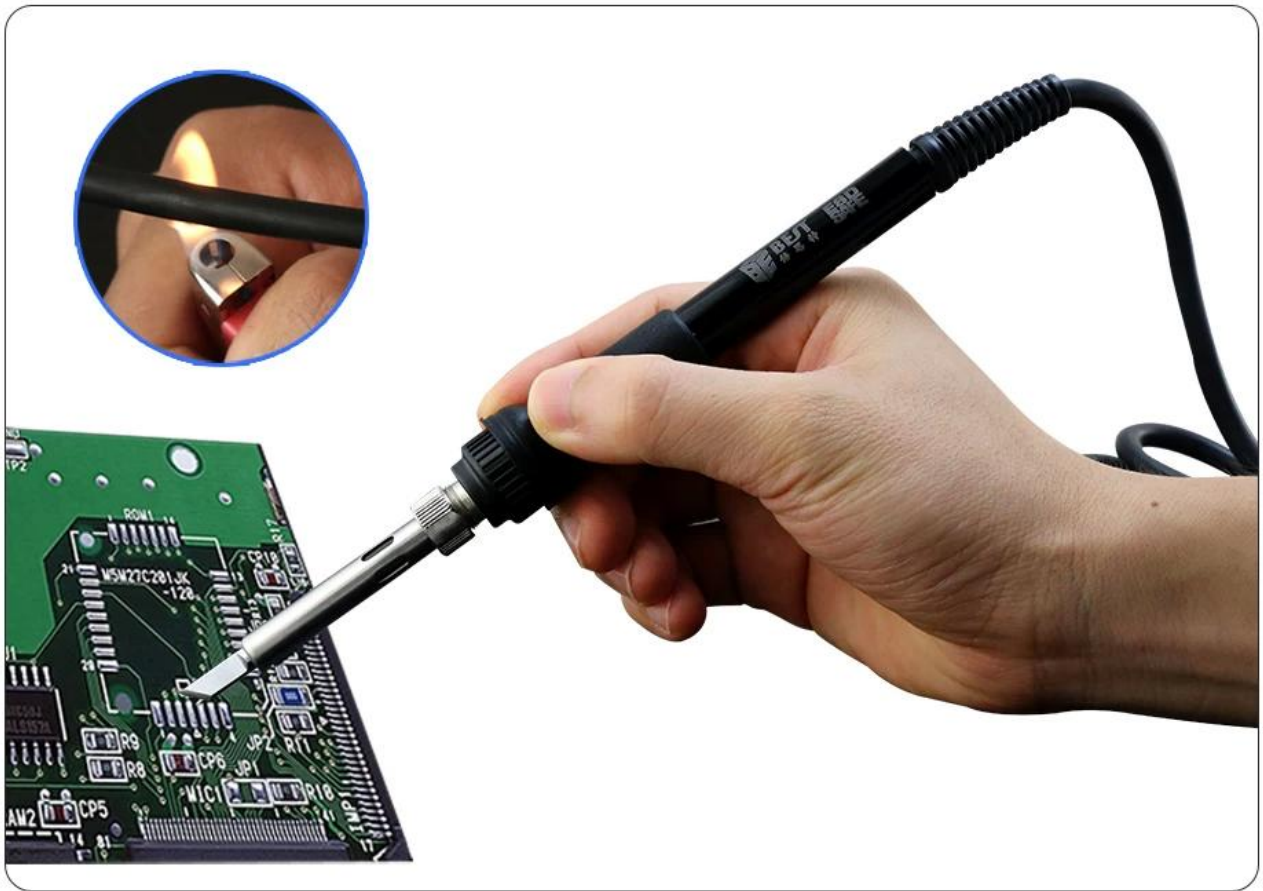

PRODUCT PACKAGING



User Manual

Thank you for purchasing the product. Please read all instructions carefully. This electronic scale is a precision instrument and should be used only on a flat, level surface. It will provide grams of relative accuracy. To ensure the most accurate results, please use the proper capacity. Operating the scale for extended periods of time may reduce the accuracy of the scale. Do not place the scale on a surface that is uneven, vibrating, or subject to strong winds. Always allow the scale to stabilize before weighing. Do not overload the scale. Always use the proper technique for placing items on the scale. Do not use the scale for weighing items that are wet, oily, or otherwise subject to evaporation. Do not use the scale for weighing items that are extremely hot or cold. Always use the scale for weighing items that are clean and dry. Always use the scale for weighing items that are at room temperature. Always use the scale for weighing items that are at a consistent weight. Always use the scale for weighing items that are at a consistent density. Always use the scale for weighing items that are at a consistent humidity. Always use the scale for weighing items that are at a consistent pressure. Always use the scale for weighing items that are at a consistent altitude. Always use the scale for weighing items that are at a consistent latitude. Always use the scale for weighing items that are at a consistent longitude. Always use the scale for weighing items that are at a consistent time zone. Always use the scale for weighing items that are at a consistent day of the week. Always use the scale for weighing items that are at a consistent month of the year. Always use the scale for weighing items that are at a consistent year of the century. Always use the scale for weighing items that are at a consistent millennium of the era. Always use the scale for weighing items that are at a consistent eon of the universe. Always use the scale for weighing items that are at a consistent epoch of the multiverse. Always use the scale for weighing items that are at a consistent aeon of the omniverse. Always use the scale for weighing items that are at a consistent era of the multiverse. Always use the scale for weighing items that are at a consistent eon of the omniverse. Always use the scale for weighing items that are at a consistent epoch of the multiverse. Always use the scale for weighing items that are at a consistent aeon of the omniverse.

I. OPERATION:

- Place scale on a horizontal flat surface. Press [ON/OFF] key to turn on the scale.
- Wait until "0.00" is displayed.
- Place the item to be weighed on the platform.
- Using the [MODE] key, you can switch between the weighing units: g, kg, and lb. Press [MODE] key to cycle through the units.
- Press [ON/OFF] key, you can turn on/off the backlight.

II. TARE WEIGHING:

- Turn the scale on as described above.
- Place the "tare item" on the platform.
- Press [TARE] and wait until "0.00" is displayed.
- Add the "net weights".

III. COUNTING FUNCTION:

- Turn on the scale and wait until the LCD displays "0.00".
- Place a sample amount (10g, 20g, 50g, or 100g), of the quantity you wish to weigh and count onto the platform.
- Press and hold [PCS] key for 2 seconds, the LCD will display a random number, for example: "03".
- Press [MODE] key to select the sample amount of material that you have put onto the platform.
- Press [PCS] key to confirm the above information, the LCD will now display "pic" in the center to show that the scale is in counting mode.
- Remove the sample quantity from the platform.
- You now can place any amount of your "count" on the scale and the LCD will display a count.
- You can switch between weighing mode and counting mode by pressing [MODE] or [PCS] key respectively.

IV. CALIBRATION:

- Reset the scale by pressing [ON/OFF] key.
- Wait until the LCD displays "0.00" and then press and hold [MODE] key for 3 seconds, the LCD will display "CAL" and then release the [MODE] key.
- Press [MODE] key again the LCD will display "CAL" followed by the required calibration weight.
- Add the required calibration weight, the display will show "PASS" and return to normal weighing mode.
- Remove the calibration weight and press [ON/OFF] to turn off the scale and the calibration is finished.

V. SPECIFICATION:

Calibration	Auto calibration
Tare range	Tare full capacity
Auto-off	20 seconds off
Operation temp.	30-80 degrees Fahrenheit
Peak	10-20,000g